

Establishing a reference range for normal canine tympanic membrane temperature measured with a veterinary aural thermometer.

This is an Accepted Manuscript of an article published by Taylor & Francis in the Veterinary Nursing Journal on 16.11.2017 available online: <https://doi.org/10.1080/17415349.2017.1377133>

Emily J. Hall MA VetMB AFHEA MRSB MRCVS (Corresponding author)

Lecturer in Veterinary Nursing Science,

School of Animal, Rural and Environmental Science,

Nottingham Trent University,

Brackenhurst,

Southwell, Nottinghamshire

NG25 0QF

Tel: 0115 8485303

Email: emily.hall@ntu.ac.uk

Emily qualified as a veterinary surgeon in 2007, and has worked in small animal first opinion practice ever since. Emily now teaches veterinary nursing students on the Foundation degree at Nottingham Trent University, and continues to work in practice at weekends.

Anne Carter BSc (Hons) MSc PhD FHEA MRSB

Senior Lecturer in Animal Science,

School of Animal, Rural and Environmental Science,

Nottingham Trent University,

Brackenhurst,

Southwell, Nottinghamshire

NG25 0QF

Anne has a PhD in canine behaviour and welfare. She continues to research in the field of canine behaviour, welfare and the canine athlete at Nottingham Trent University. Anne course leads the BSc Animal Biology at Nottingham Trent University, in addition to teaching on Anthrozoology and Animal Health & Welfare Masters courses.

Neither author has any conflicts of interest, or financial interest in this work.

Abstract

Studies have shown that tympanic membrane temperature (TMT) under reports body temperature when compared to rectal temperature. This could lead to misinterpretation of the TMT, if comparing the result to a rectal temperature range. The aim of this study was to establish a normal canine TMT reference range. 416 TMT's were taken from 157 healthy dogs, in a range of ambient temperatures. The normal reference range for canine TMT was found to be 36.6-38.8°C. This range should be considered by pet owners and veterinary professionals when interpreting TMT measured with a veterinary aural thermometer, to avoid misinterpretation of the results.

Keywords

Dog, body temperature, ear thermometer.

Introduction

In both human and veterinary medicine measuring body temperature remains an important part of any thorough clinical examination. Abnormal body temperature can indicate a range of critical conditions, so it is essential that devices used to measure body temperature are reliable and accurate. Despite considerable scientific advances in digital thermometry and thermography, rectal thermometers remain the gold standard for less-invasive body temperature measurement in veterinary patients, with pulmonary artery, oesophageal and urinary bladder temperatures providing more invasive, but true core temperature measurements. As rectal thermometry can cause stress and require additional restraint in some veterinary patients (Lamb and McBrearty, 2013) there is on-going interest in developing a reliable, less invasive method of accurately measuring body temperature. Aural thermometry remains the most promising alternative method of temperature measurement, but recent studies suggest their readings should be interpreted with caution when compared to rectal temperature reference ranges (Gomart et al., 2014; Hall and Carter, 2017; Zanghi, 2016).

There are numerous studies evaluating the use of aural thermometers in dogs, namely the animal specific PetTemp® and VetTemp® (Advanced Monitors Corporation, California, USA). TMT measurement has been shown to be better tolerated by canine patients in a veterinary setting when compared to rectal thermometry (Gomart et al., 2014, Lamb and McBrearty, 2013), suggesting that for patients where rectal thermometry is impossible due to pathology or patient temperament, TMT can provide a suitable alternative for measuring body temperature (Gomart et al., 2014; Gonzalez et al., 2002; Greer et al., 2007; Hall and Carter, 2017; Lamb and McBrearty, 2013; Rexroat et al., 1999; Southard et al., 2006; Zanghi, 2016;). Four of these studies report that TMT underestimates rectal temperature (Gomart et al., 2014; Hall and Carter, 2017; Southard et al., 2006; Zanghi, 2016) mirroring the findings of Yeoh et al. (2017) in primates. This has important implications when using TMT to measure canine body temperature as improper interpretation of the readings could result in misdiagnosis and inappropriate treatment.

The PetTemp[®] manufacturer guidelines recommend using a normal canine and feline TMT range of 37.7-39.4°C (Admon, 1999). This range is not comparable (specifically at the upper limit) to other published temperature reference ranges (see table 1). This lack of consistency defining the normal temperature range is problematic particularly for pet owners trying to interpret their own dog's body temperature. This variation could reflect the populations of animals used to define "normal canine temperature". If the dogs' temperatures were measured in a veterinary setting, rather than a familiar home environment, stress could increase the animal's body temperature, resulting in an artificially elevated temperature being incorporated into the normal range.

Table 1. Published normal canine rectal reference ranges, their sources and accessibility to pet owners.

Source	Accessibility of source	Lower temperature limit	Upper temperature limit
<i>Felder (2016)</i>	On-line veterinary manual open access	37.9°C	39.9°C
<i>Miller (2009)</i>	Textbook		39.2°C
<i>Goddard and Phillips (2011)</i>	Textbook	38.2°C	39.2°C
<i>Konietschke et al. (2014)</i>	Open access article	37.2°C	39.2 °C

The aim of this study was to determine the normal canine TMT reference range (when measured with a veterinary aural device) using healthy dogs. To provide a suitable sample size, data were pooled from previous projects measuring TMT in resting, healthy dogs. The effect of ambient temperature on TMT was also investigated.

Materials and Methods

This study and all previous projects have been approved by Nottingham Trent University's School of Animal, Rural and Environmental Science's ethics approval group.

Animals

The reference population was recruited to try and reflect the general population of pet dogs within the UK including a range of ages (juvenile to geriatric), both entire and neutered animals of both sex, half of the top 20 pedigree dog breeds in the UK (Kennel Club, 2017) and a number of crossbreeds. All animals recruited to the study were deemed to be fit and healthy by their owner, with no obvious clinical signs or recent history to suggest systemic disease; shivering dogs were not included in the reference population. If otitis externa was present in one ear, the unaffected ear was used for temperature measurement. Although a previous study has shown that there is no significant difference between the TMT measured in dog's ears with and without otitis externa (Gonzalez et al., 2002), the authors of this paper have found that excessive cerumen or aural discharge can obscure the VetTemp[®] lens and impact the accuracy. Animals with bilateral ear disease were excluded from the study. All TMT measurements were taken at rest, in a non-veterinary environment. Two study

populations were used for data collection, the first group includes pet dogs owned largely by members of staff at Nottingham Trent University. These animals were examined indoors, in a familiar environment between June 2015 and June 2017. The second study group were examined outside, prior to competing in a canicross race (dogs harnessed to their owner either running, biking or scootering over approximately 4km cross country courses) between November 2015 and April 2017. All data collection took place within the East and West Midlands, UK.

The pet dog population consisted of 32 dogs including 12 females (9 neutered) and 20 males (11 neutered), aged 6 months to 16 years (mean = 6 years). 10 breed types were represented in this sample: spaniel (n=7), cross breeds (n=6), Labrador retriever (n=5), lurcher (n=3), collie (n=3), whippet (n=2), pug (n=2), terrier (n=2), Chihuahua (n=1) and pointer (n=1). Body weight was not recorded. TMT measurements were taken in a temperature controlled environment, dogs were acclimatised to the temperature prior to thermometry.

The canicross dog population consisted of 125 dogs including 52 females (22 neutered) and 73 males (31 neutered), aged 1 -10 years old (mean = 4 years). Twenty-five breed types were represented in the sample population, the most numerous being: cross breed (n=19), pointer (n=17), collie (n=15), spaniel (n=15), lurcher (n=7), husky (n=6), Hungarian vizsla (n=5), weimaraner (n=5) other breed types (n=36). Body weight was not recorded. Ambient temperature was measured prior to TMT measurement, dogs were acclimatised to the ambient conditions prior to thermometry.

In total, the study population included 157 dogs, representing 28 breed types. Some dogs had multiple TMT measurements recorded, range 1- 9 readings per dog (mean = 3 readings per dog). For dogs with multiple readings, as each TMT was recorded on a separate day, at a different ambient temperature, for the purpose of analysis each TMT was treated as a separate data point.

An additional 30 dogs were recruited at an outdoor canine event in the West Midlands, UK, held in August 2017 to validate the reference range. The dogs' TMTs were measured at rest using the same selection criteria as the main study population. The validation population included 10 females (4 neutered) and 20 males (10 neutered), aged 5.5 months to 14 years (mean = 5 years) and included 14 breed types.

Ambient conditions

Prior to TMT measurement, ambient temperature was recorded. Measurements were taken using a HI 9564 Thermo Hygrometer (Hanna Instruments Ltd, Bedfordshire, UK).

Tympanic membrane temperature measurement

Four new VetTemp[®] VT-150 Instant Ear Thermometers (Advanced Monitors Corporation, California, USA) were used to measure TMT, as per manufacturer's instructions (see Figure 1) covered by a single use VetTemp[®] DPC-500 probe cover (Advanced Monitors Corporation, California, USA). The VetTemp[®] thermometer measures body temperatures between 32.2-43.3°C, with an accuracy of $\pm 0.2^\circ\text{C}$, within ambient temperatures of 0-40°C. All thermometers were tested reading the surface temperature of a water bath filled with opaque liquid (in an attempt to mimic the surface of the tympanic membrane), and were found to read within $\pm 0.2^\circ\text{C}$ of 36.0°C, 37.0°C and 38.0°C.



Figure 1. A VetTemp[®] aural thermometer in use.

All TMT readings were performed by the same investigator, following a standardised method used to examine animals in veterinary practice. Ears used for measurement were chosen based on presentation and restraint of the dog, to reflect the likely situation in practice. Operator accuracy was not formally assessed as part of this study.

Statistical analysis

Statistics were calculated using SPSS 23.0 (SPSS Inc., Chicago, USA). The two populations of dogs were first analysed separately, both populations were found to have a non-parametric distribution and were compared using a Mann-Whitney test, correlation was tested using Spearman Ranked correlation. The TMTs were then analysed to determine the reference interval, using methods described by Friedrichs et al. (2012). Significance was indicated at $P < 0.05$ for all tests. A histogram was plotted to identify potential outliers, using Dixon's range statistic to determine if outliers should be eliminated from further analysis. As the sample size was over 120 and non-parametric, the percentile method using 90% confidence limits was used to establish the reference limit (Friedrichs et al., 2012). A direct validation method was used, comparing the results from an additional 30 healthy individuals to the calculated reference interval (Friedrichs et al., 2012). More than 3 readings outside this range would be cause for rejection of the reference interval.

Results

The median indoor temperature was 21.2°C (range 19.0-21.2°C). For outdoor measurements, the median ambient temperature was 8.9°C (range 3.3-16.2°C). During the validation data collection the median temperature was 19.5°C (range 15.4-24.7°C).

108 TMT measurements were recorded from the indoor dog population, median TMT = 37.9°C (range 34.3-38.9°C). 309 TMT measurements were recorded from the outdoor dog population, median TMT = 37.7°C (range 36.2-39.1°C).

There was no significant difference between indoor versus outdoor TMT measurements ($Z = -1.679$, $P = 0.093$), therefore all data were pooled for further analysis.

The pooled data were then analysed to establish a reference range, with one outlier removed (TMT = 34.3°C) following identification using Dixon's outlier range statistic (Friedrichs et al., 2012). 416 TMT readings were used for the reference interval calculation. The reference interval for healthy canine TMT was calculated from 416 TMT readings, and was shown to range from 36.6 – 38.8°C (confidence interval [CI] = 36.5–36.7°C at the lower limit, CI = 38.8–38.9°C at the upper limit). There was no significant correlation between ambient temperature and TMT ($R_s = -0.007$, $P = 0.894$) (see figure 2). Additionally there was no significant difference between the resting TMTs of males and females ($Z = -0.578$, $P = 0.564$).

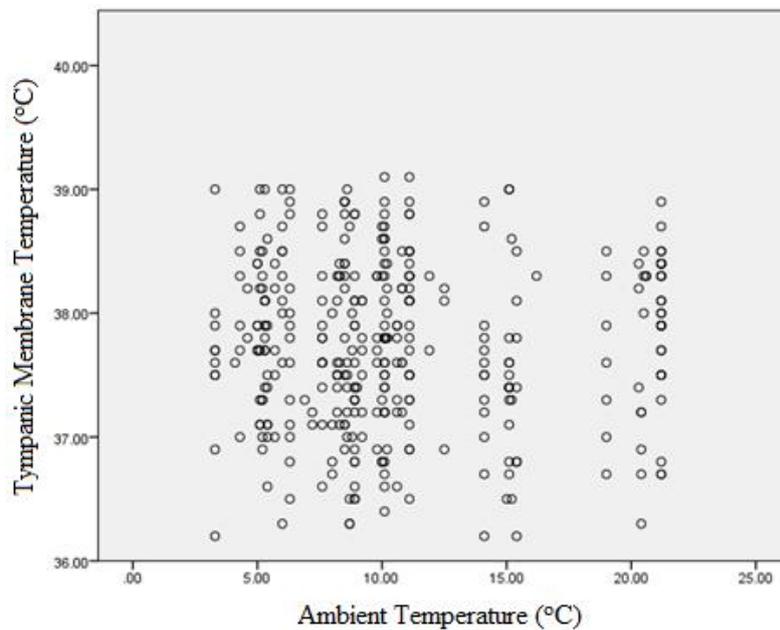


Figure 2. Scatter plot of the ambient temperature versus tympanic membrane temperature of healthy dogs.

Validation

TMT readings from the 30 dogs in the validation population all fell within this reference interval (36.6 – 38.8°C), with a median TMT of 37.9°C (range 37.0-38.5°C). The reference interval was therefore accepted.

Discussion

When measured with a veterinary aural thermometer, the normal range of TMT in healthy dogs was found to be 36.6-38.8°C. This is lower than the range of 37.7-39.4°C stated by the thermometer manufacturer (Admon, 1999). Continued use of the manufacturers recommended temperature range, or published canine rectal temperature ranges could result in hypothermia being over diagnosed, hyperthermia being missed and patients being inappropriately treated.

As the PetTemp[®] is marketed specifically to pet owners as a means of measuring their dog's temperature it is essential that owners understand how to interpret the results for their animal. Global warming is impacting the frequency of unseasonal heat waves (WMO, 2016), increasing the risk of heatstroke in all species, but particularly dogs as their ability to lose heat is quickly impaired as temperature and humidity increase (Hemmelgarn and Gannon, 2013). A dog owner may use their animal's body temperature to reach a decision about seeking veterinary advice for heat related diseases, or how to manage their animals competition or training. The reference range for canine TMT suggested in this study should reduce the likelihood of hyperthermia being missed, ensuring owners are not falsely reassured by a "normal" temperature measurement potentially putting their animal at risk.

As this study only recorded TMT, with no rectal, or core temperature measurement to compare the results to, there is a possibility some of the animals measured were not normothermic when assessed. Therefore, nothing can be said about the accuracy of the thermometry device from this study alone. Ideally, TMT would have been measured alongside rectal thermometry, however this could have affected the dog's body temperature through stress. Additionally, requiring dogs to have rectal thermometry and aural thermometry performed would have limited the number of dogs recruited to the outdoor study.

Whilst the establishment of a normal canine TMT reference range should improve the interpretation of TMT, it is important to acknowledge the limitations of TMT measurement as a clinical tool. Aural thermometers have been shown to result in more variation than rectal thermometry when operator accuracy has been investigated formally (Greer et al., 2007). This degree of inaccuracy is one of the reasons aural thermometers cannot replace rectal thermometers as the routine method of measuring body temperature in clinical patients. The tympanic membrane does not have a consistent temperature in primates (Yeoh et al., 2017), and variations between the anatomy of different dog breeds could result in a lack of consistency of probe placement. These factors could explain the reported variability of TMT when compared to rectal temperature (Lamb and McBrearty, 2013). It is also essential that the disposable probe covers are used, and changed between every patient. This not only prevents potential transmission of infections between patients, but also protects the probe from accumulation of debris which can reduce accuracy of the device (Admon, 1999).

Although the use of human aural thermometers has been investigated in dogs, the shape of the probe is considerably different to that of the veterinary specific devices (see figure 3), meaning in many dogs the human thermometer is likely to be reading the skin lining the ear canal, rather than the tympanic membrane (Greer et al., 2007). The reference range established in this study is therefore unlikely to be accurate when used to interpret results from a human ear thermometer.



Figure 3. A human aural thermometer alongside a VetTemp® aural thermometer with probe cover in place.

As this study measured TMT in a non-veterinary setting, additional work establishing a reference range in veterinary patients would be beneficial. The stress of visiting a veterinary practice can elevate body temperature, establishing how this affects the upper end of the reference range could aid veterinary professionals in interpretation of the temperature measurements.

Conclusion

The findings of this study would support a normal canine TMT reference range of 36.6-38.8°C. This is in line with previous research reporting that TMT reads approximately 0.4°C below rectal temperature (Gomart et al., 2014; Hall and Carter, 2017; Zanghi, 2016), when using a normal rectal temperature range of 37.2-39.2°C (Konietschke et al., 2014). TMT is a useful screening tool to assess body temperature in dogs; however, as TMT is not as reliable as rectal thermometry, when monitoring clinical patients TMT measurement should be followed up by rectal thermometry should hypo- or hyperthermia be detected.

References

- Admon, (1999). Your Pet's Temperature. Retrieved from <http://www.admon.com/your-pets-temperature/>
- Felder, S.E. (2016). Normal Rectal Temperature Ranges. Retrieved from MSD Veterinary Manual: <http://www.msdtvetmanual.com/appendixes/reference-guides/normal-rectal-temperature-ranges#v3362308>
- Friedrichs, K. R., Harr, K. E., Freeman, K. P., Szladovits, B., Walton, R. M., Barnhart, K. F. and Blanco-Chavez, J. (2012). ASVCP reference interval guidelines: determination of de novo reference intervals in veterinary species and other related topics. *Veterinary Clinical Pathology*, 41, 441–453. doi:10.1111/vcp.12006
- Goddard, L. and Phillips, C. (2011). Observation and assessment of the patient. In, B. Cooper, E. Mullineaux and L. Turner (Eds.), *BSAVA Textbook of Veterinary Nursing, 5th Edition* (pp. 376). Gloucester; BSAVA.
- Gomart, S. B., Allerton, F. J. W. and Gommeren, K. (2014). Accuracy of different temperature reading techniques and associated stress response in hospitalised dogs. *Journal of Veterinary Emergency and Critical Care*, 24, 279-285. DOI: 10.1111/vec.12155.
- Gonzalez, A. M., Mann, F. A., Preziosi, D. E., Meadows, R. L. and Wagnermann, C. C. (2002). Measurement of body temperature by use of auricular thermometers versus rectal thermometers in dogs with otitis externa. *Journal of the American Veterinary Medical Association*, 221, 378–380. DOI: 10.2460/javma.2002.221.378.
- Greer, R.J., Cohn, L.A., Dodam, J.R., Wagner-Mann, C.C. and Mann, F.A. (2007). Comparison of three methods of temperature measurement in hypothermic, euthermic and hyperthermic dogs. *Journal of the American Veterinary Medical Association*, 230, 1841-1848 DOI: 10.2460/javma.230.12.1841
- Hall, E.J. and Carter, A. (2017). Comparison of rectal and tympanic membrane temperature in healthy exercising dogs. *Comparative Exercise Physiology*, 13, 37-44 DOI: 10.3920/CEP160034
- Hemmelgarn, C. and Gannon, K. (2013). Heatstroke: Thermoregulation, Pathophysiology and Predisposing Factors. *Compendium: Continuing Education for Veterinarians*, E1-E7. Retrieved from <http://www.vetfolio.com/emergency-medicine/heatstroke-thermoregulation-pathophysiology-and-predisposing-factors>
- Konietschke, U., Kruse, B. D., Muller, R., Stockhaus, C., Hartmann, K. and Wehner, A. (2014). Comparison of auricular and rectal temperature measurement in normothermic, hypothermic, and hyperthermic dogs. *Tierärztliche Praxis Kleintiere*, 42, 13-19. ISSN: 1434-1239.
- Lamb, V. and McBrearty, A. R. (2013). Comparison of rectal, tympanic membrane and axillary temperature measurement methods in dogs. *Veterinary Record*, 173, 524-528. DOI: 10.1136/vr.101806.
- Miller, J. B. (2009). Hyperthermia and fever. In D.C. Silverstein and K. Hopper (Eds.), *Small Animal Critical Care Medicine* (pp. 21-26). Missouri: Saunders-Elsevier.

Rexroat, J., Benish, K. and Fraden, J. (1999). Clinical Accuracy of Vet-Temp™ Instant Ear Thermometer Comparative Study with Dogs and Cats. Advanced Monitors Corporation. Retrieved from: <http://www.admon.com/wp-content/uploads/2010/09/Humane-S°C iety-White-Paper.pdf>

Southward, E. S., Mann, F. A., Dodam, J. and Wagner-Mann, C. C. (2006). A comparison of auricular, rectal and pulmonary artery temperature in dogs with anaesthesia induced hypothermia. *Journal of Veterinary Emergency and Critical Care*, 16, 172–175. DOI: 10.1111/j.1476-4431.2005.00158.x.

The Kennel Club, (2017). Top twenty breeds in the registration order for the years 2015 and 2016. Retrieved from https://www.thekennelclub.org.uk/media/1098176/top_20_breeds_2015_-_2016.pdf

World Meteorological Organization (WMO), (2016). Provisional WMO Statement on the Status of the Global Climate in 2016. Retrieved from <https://public.wmo.int/en/media/press-release/provisional-wmo-statement-status-of-global-climate-2016>

Yeoh, W. K., Lee, J. K. W., Lim, H. Y., Gan, C. W., Liang, W., and Tan, K. K. (2017). Revisiting the tympanic membrane vicinity as core body temperature measurement site. *PLoS ONE*, 12, e0174120. DOI: 10.1371/journal.pone.0174120

Zanghi, B.M. (2016). Eye and Ear temperature using infrared thermography are related to rectal temperature in dogs at rest of with exercise. *Frontiers in Veterinary Science*, 3: 1-9. DOI: 10.3389/fvets.2016.00111